



Università degli Studi Mediterranea di Reggio Calabria
Archivio Istituzionale dei prodotti della ricerca

On the Optimal Matching Medium and the Working Frequency in Deep Pelvic Hyperthermia

This is the peer reviewed version of the following article:

Original

On the Optimal Matching Medium and the Working Frequency in Deep Pelvic Hyperthermia / Bellizzi, G.G., Sumser, K., Bevacqua, M.. - In: IEEE JOURNAL OF ELECTROMAGNETICS, RF AND MICROWAVES IN MEDICINE AND BIOLOGY.. - ISSN 2469-7249. - 5:3(2021), pp. 223-230. [10.1109/JERM.2020.3047980]

Availability:

This version is available at: <https://hdl.handle.net/20.500.12318/119085> since: 2022-12-07T14:59:31Z

Published

DOI: <http://doi.org/10.1109/JERM.2020.3047980>

The final published version is available online at: <https://ieeexplore.ieee.org/document/9310292>

Terms of use:

The terms and conditions for the reuse of this version of the manuscript are specified in the publishing policy. For all terms of use and more information see the publisher's website

Publisher copyright

This item was downloaded from IRIS Università Mediterranea di Reggio Calabria (<https://iris.unirc.it/>) When citing, please refer to the published version.

(Article begins on next page)

ON THE OPTIMAL MATCHING MEDIUM AND THE WORKING FREQUENCY IN DEEP PELVIC HYPERTHERMIA

Gennaro G. Bellizzi, Kemal Sumser, and Martina T. Bevacqua*

Abstract - A necessary step when designing electromagnetic-based medical devices is the choice of an optimal matching medium, standing between the patient and the phased array applicator, and the operating frequency. This is crucial to improve the efficiency both from a technical and clinical points of view. In this paper, we propose a new approach, based on the propagation theory, to support the selection of the matching medium properties and the working frequency in a robust way by accounting for patient body shape and properties variability. The case of adjuvant hyperthermia treatment administered to patient with tumors in the pelvic region has been used as a numerical assessment in both 2D and 3D patient specific models. For this case, the proposed approach suggests an optimal range of working frequencies ($130\text{MHz} < f < 500\text{MHz}$) and of matching material properties ($\epsilon_b < 20$), wherein one can select the working conditions depending on the trade-off between penetration and focal spot dimensions as well as other specific requirements. Results have been compared to the working frequencies used by the commercial applicators and using demineralized water as matching material. In conclusion, this work assesses the proposed approach in its general-purpose mathematical formulation, thus, paving the way for its wide application.

Keywords —**Electromagnetic Propagation Theory; Matching Material; Medical Device; Microwave Hyperthermia; Transmission Line Theory.**

I. INTRODUCTION

THE use of electromagnetic (EM) waves for medical device development is gaining a central role as from the EM versatility of serving different purposes ranging from diagnostics [1]-[3], (thermal) therapy [4]-[7] and monitoring [8]-[10]. Propagation and interaction of EM waves with biological media represents the common ground amongst all of these applications. Although it would be advisable to take advantage of EM propagation theory to optimally determine the working condition of medical devices, optimal design choices have been sometimes hampered by both technological and biocompatibility issues. Moreover, very few studies exist in which the matching media (positioned between the medical device and the patient body) and the working frequency are appropriately optimized.

The presence of the matching media aims both at reducing

This is the post-print version of the following article: G. G. Bellizzi, K. Sumser and M. T. Bevacqua, "On the Optimal Matching Medium and the Working Frequency in Deep Pelvic Hyperthermia," in IEEE Journal of Electromagnetics, RF and Microwaves in Medicine and Biology, vol. 5, no. 3, pp. 223-230, Sept. 2021, doi: 10.1109/JERM.2020.3047980. Article has been published in final form at: <https://ieeexplore.ieee.org/document/9310292>.

2469-7257 2020 IEEE Personal use of this material is permitted. Permission from IEEE must be obtained for all other uses, in any current or future media, including reprinting/republishing this material for advertising or promotional purposes, creating new collective works, for resale or redistribution to servers or lists, or reuse of any copyrighted component of this work in other works.

multi-path reflections and at maximizing the amount of EM waves transmitted inside the patient body. This directly impacts the scattered signal amplitude for diagnostic and monitoring purposes as well as it has a direct impact on the power deposition levels needed for therapy. Accordingly, the selection of the optimal matching media should be the result of a trade-off between mechanical and chemical properties (e.g., robustness, cooling capabilities, toxicity of the material), electromagnetic properties (e.g., electrical permittivity and conductivity) and actual feasibility. Generally, in thermal therapy applications, demineralized water is adopted as matching medium due to its biocompatibility [11]. Moreover, through circulation, such a matching media acts as a cooling agent preventing skin burns in therapeutic application. Also, demineralized water is generally used for its low electric conductivity (in the mS/m range) which is a mandatory requirement to reach the therapeutic field intensity and power deposition level into the tumor while not using oversized power amplifiers. However, only few studies investigated whether the above medium represents an optimal choice for EM thermal therapy.

Besides the matching media, the choice of the working frequency is essential in EM-based medical device development. The optimal working frequency is usually determined as a trade-off between penetration depth and either spatial resolution, when in diagnostic mode, or focus size, when in therapeutic mode. As a matter of fact, one would aim at a higher resolution when making a diagnosis and at a target conformal heating pattern when administering

a thermal treatment.

The selection of both frequency and matching media EM properties cannot be performed in an unrelated way and it has a direct impact on the performance of the EM-based medical device, which usually consists of a phased antenna array. In this respect, it would be advisable to address this issue starting from the EM propagation theory and then taking into consideration other specifications, such as mechanical and biocompatibility factors.

Different contributions have been proposed in the literature on the topic. Recently, Trefnà et al. [12] has proposed an innovative matching media manufacturing approach improving stability and reproducibility needed during treatments as well as for simulation purposes. However, water electrical properties have been used as matching medium. Earlier, an effective approach has been proposed to optimally determine the matching liquid electrical properties and operating frequencies for breast cancer imaging and brain strokes diagnostic purposes [13]-[15]. Although promising, generalization and application to the case of therapeutic purposes as well as actual feasibility have never been pursued. Other researchers have proposed intrinsically limited and biased trial-and-error procedures based on a posteriori observation and empirical experiences [16].

In this paper, we aim at 1) expanding and generalizing the approaches proposed in [13]-[15] for breast and brain medical diagnosis to both the case of therapeutic and diagnostic use of EM-based medical devices; 2) including patient body variability by means of a Monte-Carlo style approach which is completely missing in [13]-[15]. This is a crucial aspect that makes the selection of the working conditions much more robust and reliable. More in details, the approach does not presume to declare in absolute the optimal frequency and the matching medium combination. It aims instead at identifying convenient regions wherein one can select the working condition of the EM devices, by considering not only the good trade-off between penetration and resolution, but also other specifications (for instance, a liquid medium).

The proposed methodology is assessed for the case of adjuvant hyperthermia for patient with tumor in the pelvic region being treated with the BSD2000-3D/MR system (PYREXAR Medical, West Valley City, UT, USA) [17]. Hyperthermia treatment planning (HTP) is performed to 2D and 3D patient specific CAD models and the results compared to commercially available applicators and their corresponding working conditions.

II. THE PROPOSED APPROACH

The proposed approach benefits from the interaction mechanism between EM waves and the patient body, as well as the propagation theory. In particular, three factors are taken into account: the reflection (or alternatively transmission) coefficient, the penetration depth and the spatial resolution. The reflection coefficient represents the amount of incident EM wave which is reflected by the

biological tissues. The penetration depth is a measure of how deep the EM waves can penetrate into biological tissues, while the resolution influences the accuracy of the diagnosis and monitoring, as well as the EM field focus size in the therapy.

All of these factors have to be appropriately optimized in order to ensure a sufficient EM signal level within the tissues, which implies a precise and accurate diagnosis, monitoring or thermal treatment. To this end, in this paper, starting from the results in [13]-[15], we propose an approach composed of four different steps, as detailed in the following.

1) *1D planar layers model*. The first step consists of schematizing the interaction between the EM waves and the patient tissues by means of a one-dimensional (1D) model [18]-[20]. This consists of a sequence of planar layers, representing the different tissues, and having the same electromagnetic properties and 1D dimension of the corresponding tissue. Although simple, this 1D model can be adopted to study the EM wave propagation through the biological tissue and provide some interesting guidelines for the selection of the optimal working conditions [13]-[15].

2) *Transmission line model*. By using the formalism of transmission line [18], each planar layer is seen as an equivalent transmission line with given characteristic impedance and length, depending on the EM properties and size of the layer. In particular, by denoting with ϵ_x , σ_x and Δ_x the relative permittivity, conductivity and size of the layer mimicking a generic tissue, respectively, the characteristic impedance is evaluated as:

$$Z_x(f, \epsilon_x, \sigma_x) = \sqrt{\frac{\mu_0}{\epsilon_0 \left[\epsilon_x(f) - j \frac{\sigma_x(f)}{\omega \epsilon_0} \right]}} \quad (1)$$

while its propagation constant as:

$$k_x(f, \epsilon_x, \sigma_x) = \omega \sqrt{\mu_0 \epsilon_0 \left[\epsilon_x(f) - j \frac{\sigma_x(f)}{\omega \epsilon_0} \right]} \quad (2)$$

wherein $\omega = 2\pi f$, being f the working frequency.

3) *Estimation of the amount of reflected EM waves*. Once the biological scenario at hand is schematized by means of subsequent transmission lines, the amount of incident EM waves which is reflected by the biological tissues is analytically estimated by using the Telegraphists' equations [18]. In particular, the amplitude of the reflection coefficient $|\Gamma|$ is evaluated as a function of frequency and of the electrical properties of the matching fluid, that is [18]:

$$|\Gamma|(f, \epsilon_b, \sigma_b) = \left| \frac{Z_{eq}(f, \epsilon_x, \sigma_x, \Delta_x) - Z_b(f, \epsilon_b, \sigma_b)}{Z_{eq}(f, \epsilon_x, \sigma_x, \Delta_x) + Z_b(f, \epsilon_b, \sigma_b)} \right| \quad (3)$$

wherein the subscript b is associated to the matching medium, Z_b is the characteristic impedance associated to the matching medium and Z_{eq} is the input (or equivalent) impedance at the first interface met by EM waves, that is the one between the matching medium and the outer biological

tissue of the anatomical model. Note that Z_{eq} and Z_b must be evaluated by taking into account that both the matching medium and the tissue can be lossy. By changing the frequency f and the electromagnetic properties (ϵ_b, σ_b) of the matching fluid, a design map $|\Gamma|$ can be obtained.

As far as the EM properties (ϵ_x, σ_x) of the biological tissues, different databases, arising from ex-vivo measurements, are available in literature [21]. Moreover, effective methods have been introduced for an accurate and patient specific estimation of the in-vivo EM tissue parameters [22]-[25]. On the other hand, no systematic databases or methods exist for the estimation of the thickness Δ_x which is associated to each layer mimicking biological tissues. However, tissue's extensions variability cannot be neglected as in [13]-[15]. Indeed, the design map $|\Gamma|$ depends on Δ_x through the input impedance Z_{eq} , hence, different design maps $|\Gamma|$ can be obtained by varying the extension of the tissues Δ_x .

4) *Accounting for tissues size variability.* A Monte-Carlo-based analysis is included to take into account for thickness Δ_x variability [26]. First, a domain of possible and admissible values for each tissue has been defined [27]-[30]. Second, some values are generated as uniformly distributed random numbers over the defined domain, thus generating different vectors of possible realizations, that is $\underline{\Delta}_i = \{\Delta_b, \Delta_1, \dots, \Delta_n, \dots, \Delta_N\}$, wherein the subscripts n and i identify, respectively, the n -th tissue and the i -th realization, and N is the total number of tissues adopted in the adopted anatomical model. Then, for each i -th realization, a deterministic computation of the $|\Gamma|$ map is performed, thus generating the i -th map $|\Gamma|_i(f, \epsilon_b, \sigma_b, \underline{\Delta}_i)$. The results are finally combined by evaluating the mean $|\Gamma|_m(f, \epsilon_b, \sigma_b)$ and the standard deviation $|\Gamma|_{std}(f, \epsilon_b, \sigma_b)$ of the overall maps.

Note that step 4) aims at a robust and reliable selection of the working conditions. Indeed, one can consider that low standard deviation $|\Gamma|_{std}$ indicates that the working condition is more robust with respect to tissue extension variability, as the reflection coefficient values $|\Gamma|_i$ tend to be close to the mean $|\Gamma|_m$. On the other hand, a high standard deviation $|\Gamma|_{std}$ indicates that the reflection coefficient values $|\Gamma|_i$ are spread out over a wider range and the variability of the tissue extension can have a significant impact in the actual reflection coefficient.

As a final concern, once the $|\Gamma|_m$ map is obtained for any given application, it is then possible to select the optimal relative permittivity ϵ_b , conductivity σ_b and the frequency. Obviously, the choice has to take into account for the application-specific trade-off between penetration depth and spatial resolution (both in therapy and diagnostics). Then, the optimal working condition can be selected as the one that minimizes both the mean map $|\Gamma|_m$ and the standard deviation $|\Gamma|_{std}$. Moreover, in a practical scenario, the availability of a matching medium with optimal dielectric properties at a specific frequency need to be considered.

III. OPTIMAL WORKING CONDITIONS IN DEEP PELVIC HYPERTHERMIA

Oncologic adjuvant hyperthermia takes place when the tumor temperature is elevated to 40-44°C for 60-90 min [30]-[36]. Therapeutic benefit of adjuvant hyperthermia in combination with radiotherapy and chemotherapy has been demonstrated by clinical trials [37]-[40]. In this framework, selecting the operating frequency and the electrical properties of the matching medium represents a way towards that would enable target conformal heating, higher temperatures and the possibility to undersize the power amplifiers with direct effect on costs. In conclusion, hyperthermia is a well-suited case study to prove the feasibility of our method.

Nowadays several clinical and pre-clinical phased array applicators for deep pelvic hyperthermia have been proposed. However, generally demineralized water is used as matching medium and operating frequencies are selected in the range 70 to 120MHz [40]-[42]. However, while some evidences have shown that higher frequencies would be beneficial [43], no investigation on both matching medium and operating frequency has been proposed.

A. Design map for the selection of the optimal working condition

According to Section II, the pelvis has been modelled by using $N = 3$ layers (see Fig. 1), fat, muscle and bone, respectively, and by neglecting the skin layer, as generally done in HTP [41],[44],[45]. In particular, the bone has been considered to be indefinitely extended, being the inner tissue. In order to take into account for frequency dispersion of biological tissues, their EM properties ϵ_x, σ_x (at room temperature) have been modelled according to the fourth-order Cole-Cole model [46],[47]. Note that the use of planar multi-layer and transmission line models for the selection of the optimal working conditions of HTP applicators is completely new. From the best of authors' knowledge, no intelligent selection procedure based on both planar multi-layer and transmission line models has been proposed in literature earlier.

The relative permittivity ϵ_b of the matching medium have been assumed to range, respectively, between 1-85, whereas the investigated frequency range has been fixed from 10MHz, which is in the order of the working frequency of commercial applicators, to 1GHz. Higher frequencies are possible but not convenient due to the low penetration depth in the inspected tissues. Note that not every frequency in such a range can be used for medical purposes. As far as electric conductivity of matching medium, it is highly dependent on the frequency and is correlated to the relative permittivity. However, a lossless matching would be of interest in order to reach the therapeutic field intensity and power deposition level into the tumor while not using oversized power amplifiers. To account for a realistic matching medium, in the following, both 0 S/m and 0.04S/m have been considered.

Figure 2 depicts the results of this analysis obtained by considering 400 possible realizations of $\underline{\Delta}_i$. In particular,

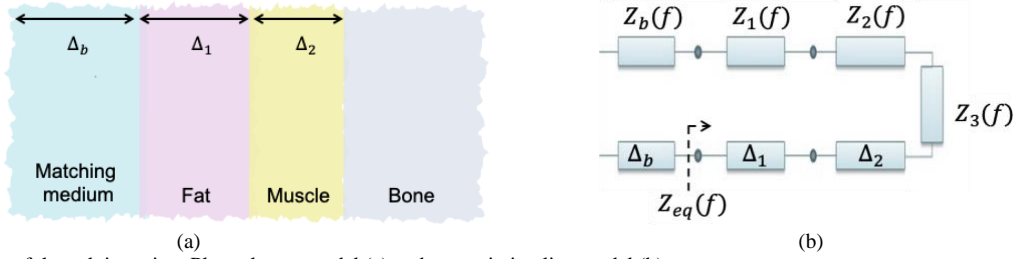


Figure 1. 1D models of the pelvic region. Planar layers model (a) and transmission line model (b).

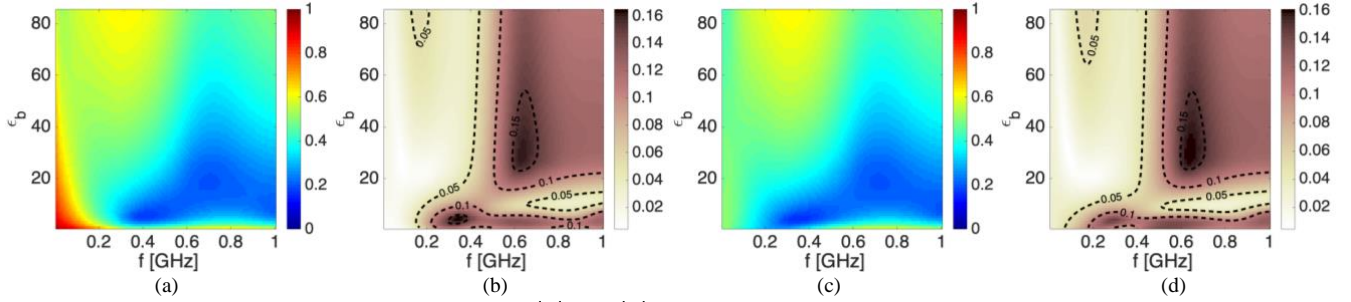


Figure 2. Optimal working conditions for deep hyperthermia. $|\Gamma|_m$ and $|\Gamma|_{std}$ maps as a function of frequency f and relative permittivity ϵ_b of the matching medium, in case of $\sigma_b = 0$ S/m (a)-(b) and $\sigma_b = 0.04$ S/m (c)-(d), respectively. As the amplitude of $|\Gamma|_m$ assumes values in the interval $[0,1]$, the scale has been set up consequently. In (b) it is not possible to see a maximum red region, as there is no region with $|\Gamma|_m$ equal to 1.

Figures 2(a) and (c) depict the $|\Gamma|_m$ for 0 S/m and for 0.04S/m, respectively. Both maps show the existence of *forbidden* regions (in red and green), wherein the reflection coefficient assumes values higher than 0.5. This means that a significant amount of the EM waves is reflected by the interface between the matching medium and the first biological tissue. On the other hand, regions corresponding to minimum values of $|\Gamma|_m$ exist lower than 0.4 (the ones in blue and light blue), in the following referred as *convenient* or *optimal* one. In figures 2(b) and (d) the $|\Gamma|_{std}$ maps are reported. These maps show that the maximum error that can be made is equal to 0.16, while it can be also lower than 0.05.

Once the convenient regions are identified through the maps, the optimal working condition can be selected as the (f, ϵ_b) pair which corresponds to a minimum value of $|\Gamma|_m$ and $|\Gamma|_{std}$, as well as which ensures a good trade-off between penetration and resolution. Possibly, other specifications can be taken into account.

Figure 2(c) identifies optimal frequency range [130–500] MHz and optimal relative permittivity ϵ_b lower than 20. Also, this range is optimal from the point of view of reliability and robustness with respect to Δ_x variability (see Fig. 2(d)). It is worth noting that the working conditions identified by the proposed approach are sensibly different to the one commonly used by the commercially available applicators. These latter rely on demineralized water (with relative permittivity about 80) as matching material and an operating frequency in the range [70-120] MHz.

Finally, it is important to stress that the thus obtained design maps represent a useful tool for the selection of the optimal working conditions. They allow to identify forbidden and convenient regions, but they do not declare in absolute the optimal (f, ϵ_b) pair. Indeed, its selection can also depend on other specifications. For instance, a liquid medium can be of interest in order to fill the entire space

between body and the applicator. Then, among the different pairs (f, ϵ_b) belonging to the convenient region, one can select the one that allows to implement a liquid medium.

B. 2D Proof-of-Concept Analysis

A 2D proof-of-concept analysis has been carried out by using an in-house developed MoM considering a slice of a patient with a tumor in the pelvis region. The 2D model [22] has been considered to be placed in front of a line source with a distance of 0.38 m from the center of the model.

The aim of these numerical analysis is to solve the forward problem and compute the induced current distributions, when different working conditions are considered. First, the state-of-the-art case of demineralized water as matching medium using 70MHz, 100MHz, 120MHz has been considered. Second, these latter have been benchmarked to the working conditions as determined from the proposed approach. For instance, three different frequencies belonging to the convenient regions have been considered, that are 128MHz, 250 MHz and 434 MHz. Each frequency has been tested by using a matching media having ϵ_b higher as well as lower than 20.

Figure 3 depicts the amplitudes of the currents induced in the pelvis in different working conditions. In particular, as the frequency is different for each working condition, in order to have a fair comparison, the current have been normalized with respect to the energy of the corresponding incident field. In the following, this quantity is referred as \hat{W} . As long as the frequency is lower than 130 MHz, the penetration depth is sufficiently large, so that the EM wave can penetrate the tissues. However, the induced currents have a very low amplitude, unless the right matching fluid is

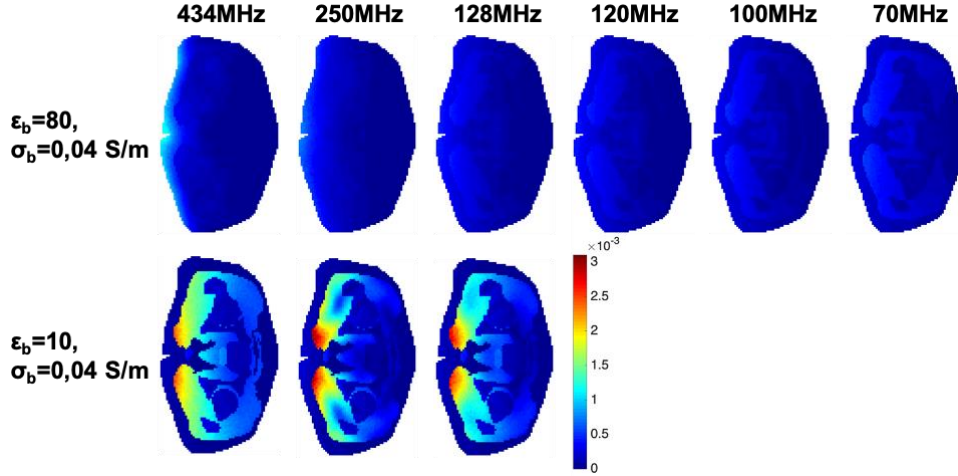


Figure 3. 2D assessment of the optimal working conditions for deep HTP. Amplitudes of induced currents normalized with respect to the energy (l_2 -norm) of the incident fields, as a function of the working frequency and the properties of the matching medium. The line source is located at the left side of the pelvis.

adopted. When a frequency higher than 128 MHz is considered, the selection of the matching fluid plays a key role. Indeed, in the case of 250MHz and 434 MHz, and $\epsilon_b = 80$, the EM wave cannot penetrate the tissues, as the working conditions correspond to the forbidden region in Figure 2(c). On the other hand, when the right matching fluid is adopted, currents with larger amplitude are induced in the tissues.

Table I reports the energy (l_2 -norm) of \widehat{W} over the investigation domain of the normalized currents, thus further confirming a higher energy level is reached if the working conditions are selected according to Subsection III.A.

Freq [MHz]	70	100	120	128	128	250	250	434	434
ϵ_b	80	80	80	80	10	70	10	80	10
$\ \widehat{W}\ [10^{-4}]$	2.3	2.0	1.9	2	32	2.4	26	3.8	28

Table I. Energy of the normalized currents \widehat{W} as a function of the working frequency and the properties of the matching medium ($\sigma_b = 0.04 S/m$).

IV. IMPACT ON DEEP PELVIC HTP

A. The Patient Model

The 3D patient model having a solid tumor in pelvis region has been created using the clinical segmentation procedure. This procedure is based on delineation of computerized tomography (CT) scans into normal tissues and the target volume using a semi-automatic segmentation routine followed by a manual adjustment in software tool iSeg (Zurich Medtech, Zurich, Switzerland). The CT scans have been taken when the patient is lying in a tailored sling (PYREXAR Medical, West Valley City, Utah) matching patient positioning and body shape during treatment [33]. A trained clinician has identified the hyperthermia target volume (HTV) starting from the clinical target volume (CTV) for radiotherapy treatment, and adding certain margins depending on the specific case [48]-[50].

B. The HTP Workflow

The first step for HTP has included importing the segmented 3D patient model into Sim4Life (Zurich MedTech AG, Zurich, Switzerland) along with a 3D applicator model, the Pyrexar BSD2000 3D/MRI (Sigma Eye) applicator (PYREXAR Medical, West Valley City, UT, USA). Electromagnetic tissues properties for these frequencies have been assigned to each of the segmented tissues [21]. The total field has been computed for a 1V sinusoidal signal excitation and 20 periods of harmonic signal for each antenna at the operating frequency. The electric field per antenna has been normalized to 1W radiated power and the cubic filtered SAR (cf-SAR) pattern optimized using our *Visualisation Tool for Electromagnetic Dosimetry and Optimisation* (VEDO) software [50].

The adopted optimization strategy aims at maximizing the Target to Hotspot Quotient (THQ) defined as the ration between the average SAR within the target volume and the average SAR at the hot-spot, which is defined as the cumulative 1% volume in all healthy tissues with the highest SAR [51]. The Particle Swarm Optimization scheme has been used to maximize the THQ cost function.

C. Comparative Assessment

In order to assess the finding of the proposed approach, we have compared the outcome of HTP, on the same patient model, under different working conditions mimicking actual design choice performed by different applicators meant to treat tumor in the pelvic area [17],[40],[52]. To this end, we have considered five different cases. First, the case of demineralized water as matching media and operating frequency equal to 70MHz, 100MHz and 120MHz have been simulated. In this case, relative permittivity has been set equal to 79.08 and conductivity equal to 0.001 S/m. Second, being the system optimized to work in that range of frequencies, we have considered 128MHz and the relative permittivity equal to 10, according to the convenient region as in Section III.A. Lastly, we have considered the case of

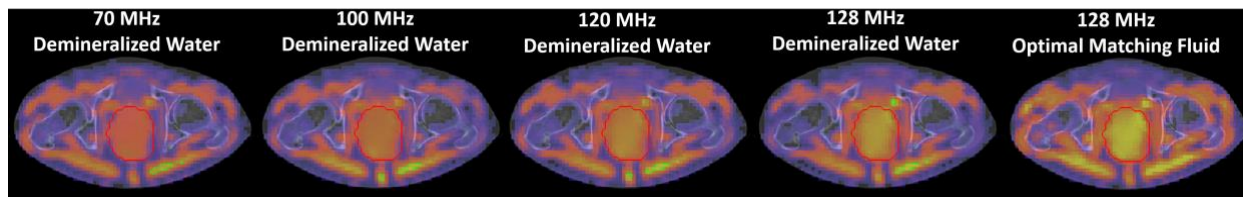


Figure 4. 3D assessment of the optimal working conditions for deep HTP. Predicted SAR distributions within the patient model as a function of the working frequency and the properties of the matching medium.

Freq [MHz]	ϵ_b	σ_b [mS/m]	THQ	TC25 [%]	TC50 [%]	TC75 [%]
70	79,086	1,14	0.49	85	2	0
100	79,086	1,14	0.57	94	11	0
120	79,086	1,14	0.62	97	32	0
128	79,086	1,14	0.66	98	46	0
128	10	1,14	0.60	99	62	1

Table II. HTP SAR quality metrics as a function of the working frequency and the properties of the matching medium.

using demineralized water as matching media while still selecting the operating frequency deemed optimal.

D. Evaluation Metrics

The different performance has been quantitatively investigated using standard HTP SAR quality metrics: THQ and target coverage (TC). These metrics are currently used for clinical decision making as they were demonstrated to be predictive for median target temperature [53]. Specifically, the THQ is defined in the previous section. The TC is the volume percentage of the hyperthermia target volume covered by the 25% (TC25), 50% (TC50), and 75% (TC75) iso-SAR contour, with SAR being normalized to the maximum SAR in the patient. The higher the coverage, the better performance the matching fluid are provided.

E. Results & Discussion

Figure 4 depicts a cut view of the SAR distribution for each of these cases. Table II reports the SAR quality metrics as well as details for all the different investigated cases. The results show that changing the frequency (70, 100 and 120MHz) while using demineralized water as matching media has the larger impact on TC25 and TC50 with an average increase of 7 percentage points (range 2-14 percentage points) and 47 percentage points (range 30-60 percentage points), respectively. On the other hand, this has a smaller impact on the THQ and TC75 which remain on average unaltered. A similar trend is observed when comparing the case of 128MHz as operating frequency and demineralized water as matching media with the case deemed optimal according to Section III.A. However, a larger impact can be observed on TC50 with an increase of 26 %-points while TC25 and TC75 remain approximately unaltered.

By increasing the frequency, better performance is obtained, and a key role is played by the matching media. Indeed, when the relative permittivity is equal to 10, a higher SAR deposition is reached, as also shown in Figure 4.

In this preliminary work, we have posed our attention only on SAR quality metrics. However, our findings are consistent also in terms of predicted temperature [53]. Earlier, through simulation studies, the considered SAR quality metrics have been demonstrated to be optimal surrogate for the temperature distributions as well as highly correlated to median predicted target temperature (T50). Accordingly, differences in these SAR quality indicators would translate into a variation in predicted HTV temperature distribution. Hence, we have chosen not to include temperature simulation for two main reasons: SAR is usually the first step of technology development as it is the more straightforward indicator of the field propagation and, moreover, blood perfusion mechanisms are not fully known. Therefore, the open debate regarding thermal properties as well as the unknown impact on the clinical outcome could lead to different interpretations of these preliminary results.

V. CONCLUSION

An innovative approach for identifying convenient regions wherein one can select the working conditions of the EM medical devices is proposed based on propagation theory and starting from works [13]-[15]. In order to make their selection more robust and reliable, the patient body variability is considered via a Monte Carlo style analysis.

Even if general purpose, the proposed procedure is tested within the framework of hyperthermia. For this specific application, the proposed method identifies [130-500] MHz as optimal range of working frequencies and a material with relative permittivity lower than 20. This optimal region has been preliminary tested in 2D simplified scenario, by showing that the amplitude of the currents induced within the tissues is increased. Then, 3D simulations have been performed in the range of [70-128] MHz, in which the used clinical system has been optimized. Still, the 3D analysis is inline with the results of simplified 2D scenario.

REFERENCES

- [1] Kosmas, P. and C.M. Rappaport, Time reversal with the FDTD method for microwave breast cancer detection. *IEEE Transactions on Microwave Theory and Techniques*, 2005. 53(7): p. 2317-2323.
- [2] N. K. Nikolova, Microwave Imaging for Breast Cancer, in *IEEE Microwave Magazine*, vol. 12, no. 7, pp. 78-94, Dec. 2011
- [3] Nn C. Kaye, I. Jeffrey and J. LoVetri, "Improvement of Multi-Frequency Microwave Breast Imaging through Frequency Cycling and Tissue-Dependent Mapping," in *IEEE Transactions on Antennas and Propagation*, vol. 67, no. 11, pp. 7087-7096, Nov. 2019.
- [4] Bellizzi G.G., Drizdal T., van Rhoon G.C., Crocco L., Isernia T., Paulides M.M. The potential of constrained SAR focusing for hyperthermia treatment planning: Analysis for the head & neck region. *Physics in Medicine & Biology*, 2018.
- [5] Kok HP, Van Haaren PM, Van de Kamer JB, Wiersma J, Van Dijk JD, Crezee J., High-resolution temperature-based optimization for hyperthermia treatment planning. *Physics in Medicine & Biology*, 2005. 50(13): p. 3127.
- [6] Dobšiček Trefná, H., J. Vrba, and M. Persson, Evaluation of a patch antenna applicator for time reversal hyperthermia. *International Journal of Hyperthermia*, 2010. 26(2): p. 185-197.
- [7] Y. Mohtashami, H. Luyen, J. F. Sawicki, J. D. Shea, N. Behdad and S. C. Hagness, "Tools for Attacking Tumors: Performance Comparison of Triaxial, Choke Dipole, and Balun-Free Base-Fed Monopole Antennas for Microwave Ablation," in *IEEE Antennas and Propagation Magazine*, vol. 60, no. 6, pp. 52-57, Dec. 2018
- [8] M. Haynes, J. Stang and M. Moghaddam, "Real-time Microwave Imaging of Differential Temperature for Thermal Therapy Monitoring," in *IEEE Transactions on Biomedical Engineering*, vol. 61, no. 6, pp. 1787-1797, June 2014.
- [9] Lopresto V, Pinto R, Farina L, Cavagnaro M., Microwave thermal ablation: effects of tissue properties variations on predictive models for treatment planning. *Medical engineering & physics*, 2017. 46: p. 63-70.
- [10] Goldberg SN, Gazelle GS, Solbiati L, Livraghi T, Tanabe KK, Hahn PF, et al, Ablation of liver tumors using percutaneous RF therapy. *American journal of roentgenology*, 1998. 170(4): p. 1023-1028.
- [11] Sumser, K.; Bellizzi, G.G.; van Rhoon, G.C.; Paulides, M.M., "The Potential of Adjusting Water Bolus Liquid Properties for Economic and Precise MR Thermometry Guided Radiofrequency Hyperthermia." *Sensors* 20.10, 2946, 2020.
- [12] Trefna, H.D. and A. Ström, Hydrogels as a water bolus during hyperthermia treatment. *Physics in Medicine & Biology*, 2019.
- [13] Rappaport, C., Determination of bolus dielectric constraint for optimum coupling of microwaves through skin for breast cancer imaging," *Int. J. of Antennas and Propag.*, Vol. 2008, 2008.
- [14] I. Catapano, L. Di Donato, L. Crocco, O. M. Bucci, A. F. Morabito, T. Isernia, and R. Massa, "On Quantitative Microwave Tomography of Female Breast," *Progress In Electromagnetics Research*, Vol. 97, 75-93, 2009.
- [15] R. Scapaticci, L. Di Donato, I. Catapano, and L. Crocco, "A Feasibility Study on Microwave Imaging for Brain Stroke Monitoring," *Progress In Electromagnetics Research B*, Vol. 40, 305-324, 2012.
- [16] M. Meaney, S. A. Pendergrass, M. W. Fanning, and K. D. Paulsen, "Importance of using a reduced contrast coupling medium in 2D microwave breast imaging," *Journal of Electromagnetic Waves and Applications*, vol. 17, no. 2, pp. 333-355, 2003.
- [17] Gellermann, J.; Wlodarczyk, W.; Ganter, H.; Nadobny, J.; Föhling, H.; Seebass, M.; Felix, R.; Wust, P. A practical approach to thermography in a hyperthermia/magnetic resonance hybrid system: Validation in a heterogeneous phantom. *Int. J. Radiat. Oncol. Biol. Phys.* 61, 267-277, 2005.
- [18] Franceschetti, G., *Electromagnetics: Theory, Techniques, and Engineering Paradigms*, Springer Science & Business Media, 2013.
- [19] J. E. Roy, "New results for the effective propagation constants of nonuniform plane waves at the planar interface of two lossy media," in *IEEE Transactions on Antennas and Propagation*, vol. 51, no. 6, pp. 1206-1215, June 2003.
- [20] F. Frezza and N. Tedeschi, "On the electromagnetic power transmission between two lossy media: discussion," *J. Opt. Soc. Am. A* 29, pp. 2281-2288, 2012.
- [21] S. Gabriel, R W Lau, C. Gabriel, The dielectric properties of biological tissues: II. Measurements in the frequency range 10 Hz to 20 GHz, *Phys. Med. Biol.*, 41: 2251-2269, 1996.
- [22] Bevacqua, M.; Bellizzi, G.; Isernia, T.; Crocco, L., A method for quantitative imaging of electrical properties of human tissues from only amplitude electromagnetic data. *Inverse Problems*, 2019. 35(2): p. 025006.
- [23] Bevacqua, M.; Bellizzi, G.; Isernia, T.; Crocco, L., A method for effective permittivity and conductivity mapping of biological scenarios via segmented contrast source inversion. *Progress In Electromagnetics Research*, 2019. 164: p. 1-15.
- [24] L. M. Neira, B. D. Van Veen and S. C. Hagness, High-resolution microwave breast imaging using a 3-D inverse scattering algorithm with a variable-strength spatial prior constraint, *IEEE Trans. Antennas Propag.*, 65(11):6002-6014, 2017.
- [25] A. Arduino, O. Bottasuscio, M. Chiampi and L. Zilberti, Magnetic resonance-based imaging of human electric properties with phaseless contrast source inversion, *Inv. Probl.* 34, 084002, 2018.
- [26] Rubinstein, Reuven Y., and Dirk P. Kroese. Simulation and the Monte Carlo method. Vol. 10. John Wiley & Sons, 2016.
- [27] Bellizzi, G.G.; Sumser, K.; VilasBoas-Ribeiro, I.; Curto, S.; Drizdal, T.; Van Rhoon, G.C.; Franckena, M.; Paulides, M.M. Standardization of patient modeling in hyperthermia simulation studies: introducing the Erasmus Virtual Patient Repository., *International Journal of Hyperthermia* 37.1 (2020): 608-616.
- [28] E. Zastrow, S. K. Davis, M. Lazebnik, F. Kelcz, B. D. V. Veen and S. C. Hagness, "Development of Anatomically Realistic Numerical Breast Phantoms With Accurate Dielectric Properties for Modeling Microwave Interactions With the Human Breast," in *IEEE Transactions on Biomedical Engineering*, 55(12): 2792-2800, Dec. 2008.
- [29] Gosselin MC, Neufeld E, Moser H, et al., Development of a new generation of high-resolution anatomical models for medical device evaluation: the Virtual Population 3.0, *Physics in Medicine and Biology*, 59(18):5287-5303, 2014.
- [30] Stauffer PR, Evolving technology for thermal therapy of cancer. *International Journal of Hyperthermia*, 21(8):731-44, 2005.
- [31] J.Stang, M. Haynes, P. Carson and M. Moghaddam, "A Preclinical System Prototype for Focused Microwave Thermal Therapy of the Breast," in *IEEE Transactions on Biomedical Engineering*, vol. 59, no. 9, pp. 2431-2438, Sept. 2012.
- [32] P. T. Nguyen, A. M. Abbosh and S. Crozier, "3-D Focused Microwave Hyperthermia for Breast Cancer Treatment with Experimental Validation," in *IEEE Transactions on Antennas and Propagation*, vol. 65, no. 7, pp. 3489-3500, July 2017, doi: 10.1109/TAP.2017.2700164.
- [33] G. G. Bellizzi, L. Crocco, G. M. Battaglia and T. Isernia, "Multi-Frequency Constrained SAR Focusing for Patient Specific Hyperthermia Treatment," in *IEEE Journal of Electromagnetics, RF and Microwaves in Medicine and Biology*, vol. 1, no. 2, pp. 74-80, Dec. 2017.
- [34] G. Muntoni, A. Fanti, G. Montisci and M. Muntoni, "A Blood Perfusion Model of a RMS Tumor in a Local Hyperthermia Multi-Physic Scenario: A Preliminary Study," in *IEEE Journal of Electromagnetics, RF and Microwaves in Medicine and Biology*, vol. 3, no. 1, pp. 71-78, March 2019.
- [35] L. Xu and X. Wang, "Focused Microwave Breast Hyperthermia Monitored by Thermoacoustic Imaging: A Computational Feasibility Study Applying Realistic Breast Phantoms," in *IEEE Journal of Electromagnetics, RF and Microwaves in Medicine and Biology*, vol. 4, no. 2, pp. 81-88, June 2020.
- [36] K. R. Mahmoud and A. Montaser, "Design of Hyperthermia Applicator to Heat Multi Brain Tumors Simultaneously based on Adaptive Beamforming Technique," in *IEEE Journal of Electromagnetics, RF and Microwaves in Medicine and Biology*, doi: 10.1109/JERM.2020.3015345.
- [37] Niloy R. Datta, Susanne Rogers, Dirk Klingbiel, Silvia Gómez, Emsad Puric & Stephan Bodis, Hyperthermia and radiotherapy with or without chemotherapy in locally advanced cervical cancer: a systematic review with conventional and network meta-analyses. *International Journal of Hyperthermia*, 2016. 32(7): p. 809-821.
- [38] Niloy R. Datta, Susanne Rogers, Silvia Gómez Ordóñez, Emsad Puric & Stephan Bodis, Hyperthermia and radiotherapy in the management of head and neck cancers: A systematic review and meta-analysis. *International Journal of Hyperthermia*, 2016. 32(1): p. 31-40.
- [39] Van den Tempel, N.; Laeber, C.; Odijk, H.; van Cappellen, W.A.; van Rhoon, G.C.; Franckena, M.; Kanaar, R., The effect of thermal dose on hyperthermia mediated inhibition of DNA repair through

homologous recombination. *Oncotarget*, 8(27): p. 44593-44604, 2017.

- [40] Turner, P.F., A. Tumei, and T. Schaefermeyer, BSD-2000 approach for deep local and regional hyperthermia: physics and technology. *Strahlenther Onkol.*, 165(10): p. 738-741, 1989.
- [41] Mulder HT, Curto S, Paulides MM, et al., Systematic quality assurance of the BSD2000-3D MR-compatible hyperthermia applicator performance using MR temperature imaging. *International Journal of Hyperthermia*, 35(1): p. 305-313, 2018.
- [42] R. Zweije, H. P. Kok, A. Bakker, A. Bel and J. Crezee, "Technical and Clinical Evaluation of the ALBA-4D 70MHz Loco-Regional Hyperthermia System," *2018 48th European Microwave Conference (EuMC)*, Madrid, 2018, pp. 328-331.
- [43] Bastien Guérin, Jorge F. Villena, Athanasios G. Polimeridis, Elfar Adalsteinsson, Luca Daniel, Jacob K. White, Bruce R. Rosen & Lawrence L. Wald "Computation of ultimate SAR amplification factors for radiofrequency hyperthermia in non-uniform body models: impact of frequency and tumour location." *International Journal of Hyperthermia*, 34(1): 87-100, 2018.
- [44] Aklan B, Hartmann J, Zink D, et al., Regional deep hyperthermia: impact of observer variability in CT-based manual tissue segmentation on simulated temperature distribution. *Physics in Medicine & Biology*. 62(11): p. 4479, 2017.
- [45] Kok, H.P. and J. Crezee. Adaptive Treatment Planning for Locoregional Hyperthermia: A Necessary Tool for Optimizing Treatment Quality. in *2018 EMF-Med 1st World Conference on Biomedical Applications of Electromagnetic Fields (EMF-Med)*, 2018.
- [46] Gabriel, S., R. W. Lau, and C. Gabriel, "The dielectric properties of biological tissues: 3. Parametric models for the dielectric spectrum of tissues," *Phys. Med. Biol.*, Vol. 41, 2271-2293, 1996.
- [47] P. A. Hasgall et al., "IT'IS Database for thermal and electromagnetic parameters of biological tissues (Version 4.0)," vol. itis.swiss/database, 2018.
- [48] Burnet, N. G.; Thomas, S. J.; Burton, K. E.; Jefferies, S. J., Defining the tumour and target volumes for radiotherapy. *Cancer Imaging*, 2004. 4(2): p. 153.
- [49] Canters RA, Paulides MM, Franckena MF, van der Zee J, van Rhoon GC Implementation of treatment planning in the routine clinical procedure of regional hyperthermia treatment of cervical cancer: An overview and the Rotterdam experience. *International journal of hyperthermia*, 28(6): p. 570-581, 2012.
- [50] Rijnen Z, Bakker JF, Canters RA, Togni P, Verduijn GM, Levendag PC, et al, Clinical integration of software tool VEDO for adaptive and quantitative application of phased array hyperthermia in the head and neck. *International Journal of Hyperthermia*, 29(3): p. 181-193, 2013.
- [51] Canters RA, Wust P, Bakker JF, Van Rhoon GC., A literature survey on indicators for characterisation and optimisation of SAR distributions in deep hyperthermia, a plea for standardisation. *International Journal of Hyperthermia*, 2009. 25(7): p. 593-608, 2009.
- [52] Crezee J, Van Haaren PMA, Westendorp H, De Greef M, Kok HP, Wiersma J et al., "Improving locoregional hyperthermia delivery using the 3-D controlled AMC-8 phased array hyperthermia system: A preclinical study." *International Journal of Hyperthermia* 25(7): 581-592, 2009.
- [53] Bellizzi GG, Drizdal T, van Rhoon GC, Crocco L, Isernia T, Paulides MM, Predictive value of SAR based quality indicators for head and neck hyperthermia treatment quality. *International Journal of Hyperthermia*, 2019. 36(1): p. 456-465.



Gennaro G. Bellizzi was born in Naples, Italy, in 1992. He received the M.Sc. in biomedical engineering (summa cum laude) from the University of Naples "Federico II," in 2015, and the Ph.D. in electronic engineering (applied electromagnetism) at the University "Mediterranea" of Reggio Calabria, Reggio Calabria, Italy, in March 2019. Amongst other awards, he was the recipient of One-Day-Workshop

organization fund granted by Ambassade de France en Italie (2016), of the IEEE Antennas and Propagation Society Doctoral Research Grant (2017) and of the Young Scientist Award (2020). From 2018 to 2020, he has been with the COST Action My-Wave CA17115 as management committee substitute and working as Engineering Project Manager within the Department of Radiotherapy, Erasmus MC, Rotterdam, The Netherlands.



Kemal Sumser was born in Turkey in 1991. He received the M.Sc. degree in electrical engineering from the Middle East Technical University, Ankara, Turkey, in 2016. He is currently working towards the Ph.D. degree in the Department of Radiotherapy, Erasmus MC, Rotterdam, The Netherlands. His work is primarily on a Dutch Cancer Society project entitled: "Multi-coil magnetic resonance guided hyperthermia for precision treatment of advanced head and neck carcinoma". His research interests are in the area of hyperthermia treatment planning, multi physics modelling, and magnetic resonance imaging.



Martina Teresa Bevacqua was born in Reggio Calabria, Italy, in 1988. She received from the University Mediterranea of Reggio Calabria, Italy, the M.S. Laurea degree (summa cum laude) in electronic engineering in July 2012 and the Ph.D in Information Engineering in May 2016. She is currently working as Assistant Professor at the University Mediterranea of Reggio di Calabria and her research activity mainly concerns electromagnetic inverse scattering problems with particular interest in biomedical and subsurface noninvasive diagnostics.

Dr. Bevacqua was the recipient of the Barzilai Award from the Italian Electromagnetics Society in 2014 and Young Scientist Award during the 2018 URSI Atalantic Radio Science Meeting. Moreover, she received the Honorable Mention from IEEE-Antennas and Propagation Society (Central and Southern Italy Chapter) in the 2016 best Student Member paper competition.